

CYPRUS ORGANIZATION FOR THE PROMOTION OF QUALITY
CYPRUS ACCREDITATION BODY



ACCREDITATION CERTIFICATE no. L033-4

The Board of Governors
of the Cyprus Organization for the Promotion of Quality
acting as the authorized Cyprus Accreditation Body
according to the Article 7 of the Law 156(I)/2002

grants ACCREDITATION to the

Laboratory
SUNDIAL CO LTD – LABORATORY DIVISION

in Limassol

which has been assessed according to the Accreditation Criteria for
Calibration Laboratories as defined in the standard

CYS EN ISO/IEC 17025:2017

as **competent to perform the Methods** defined in the Scope of Accreditation referred to in the **Annex** of this certificate; the said Annex represents inextricable part of the certificate. The **Accreditation Scope** can only be modified after a decision of the Cyprus Accreditation Body.

Cyprus Accreditation Body is a signatory to the European co-operation for Accreditation (EA) Multilateral Agreement (MLA) in the above-mentioned field.

The current Accreditation Certificate, no. **L033-4**, is issued on the **15th November 2023** and is valid from **8th September 2023** until the **7th September 2027**.

Accreditation was granted for the first time on the 8th September 2011.



Antonis Ioannou
Director

Date: 15 November 2023

This laboratory is accredited in accordance with the recognised International Standard ISO/IEC 17025:2017. This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management System (ISO-ILAC-IAF Communiqué, 04/2017).



CYPRUS ORGANIZATION FOR THE PROMOTION OF QUALITY
CYPRUS ACCREDITATION BODY

Annex
to the Accreditation Certificate no. L 033-4

Scope of Accreditation
of the Laboratory
SUNDIAL CO LTD – LABORATORY DIVISION

Valid as from 8th September 2023 to 7th September 2027


Calibration & Measurement Capability (CMC)			
Measurand / Calibration Item	Range of measurements	Expanded Measurement Uncertainty (k=2)*	Remarks
Volume measurements			
Volume of pipettes	0,2 µl - 10 µl	0,03...0,2 µl	According to: CYS EN ISO 8655-6:2022 & ISO/TR 20461:2023
	> 10 µl - 100 µl	0,2....0,3 µl	
	> 100 µl....1 ml	0,3.....1 µl	
	> 1 ml - 10 ml	18 µl	

* For values of volume in between the referred ones, the uncertainty is scaled accordingly.

Authorised person to sign calibration reports is **Ms Maria Christodoulou**.

General Remarks

This Annex refers **only for calibrations** performed **in the premises of the Laboratory**, at the following address: 2, Chrysanthou Episkopou Pafou (2nd floor), CY-3022, Limassol.

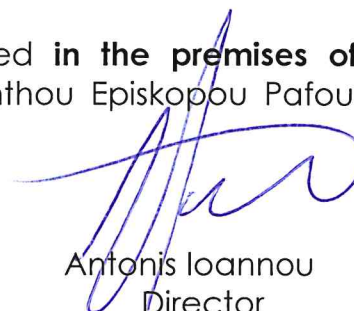

Antonis Ioannou
Director

Date: 15 November 2023