

CYPRUS ORGANIZATION FOR THE PROMOTION OF QUALITY
CYPRUS ACCREDITATION BODY



ACCREDITATION CERTIFICATE no. L117

The Board of Governors
of the Cyprus Organization for the Promotion of Quality
acting as the authorized Cyprus Accreditation Body
according to the Article 7 of the Law 156(I)/2002

grants accreditation to

MULTILAB TESTING LTD
Calibration Laboratory

in Nicosia, Cyprus

which has been assessed according to the Accreditation Criteria for
Calibration Laboratories as defined in the standard

CYS EN ISO/IEC 17025:2017

As **competent to perform the Methods** defined in the Scope of Accreditation referred to in the **Annex** of this certificate; the said Annex represents inextricable part of the certificate. The **Accreditation Scope** can only be modified after a decision of the Cyprus Accreditation Body.

Cyprus Accreditation Body is a signatory to the European co-operation for Accreditation (EA) Multilateral Agreement (MLA) in the above-mentioned field.

The current Accreditation Certificate, no. **L117**, is issued on **20th October 2023** and is valid from the **13th January 2022** until the **12th January 2026**.

Accreditation was granted for the first time on the 13th January 2022.


Antonis Ioannou
Director

Date: 20 October 2023

This laboratory is accredited in accordance with the recognised International Standard ISO/IEC 17025:2017. This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management System (ISO-ILAC-IAF Communiqué, 04/2017).



Annex
of the Accreditation Certificate number L117

Scope of Accreditation
of
MULTILAB TESTING LTD
Calibration Laboratory

Valid as from the 13th January 2022 until the 12th January 2026.


Calibration & Measurement Capability (CMC)			
Measurand / Calibration item	Range of measurement	Expanded Measurement Uncertainty (k=2)¹	Remarks
Pressure Measurements			
Pressure (relative) / Analog and digital gauge pressure measuring instruments of direct reading	1 bar to 700 bar	0,25 %	Oil or water medium. According to guide DKD-R 6-1 (2014) Calibration can also be performed on-site
	-0,95 bar to -0,1 bar	0,5 %	Gas pressure medium. According to guide DKD-R 6-1 (2014) Calibration can also be performed on-site
	5,0 mbar to 25,0 mbar	0,5 %	
	0,1 bar to 10 bar	0,25 %	
	10 bar to 200 bar	0,5 %	
Pressure (absolute) / Analog and digital gauge pressure measuring instruments of direct reading	0,9 bar to 7 bar	0,1 %	Gas pressure medium. According to guide DKD-R 6-1 (2014)

¹ Where Expanded Measurement Uncertainty is expressed without the corresponding units, it denotes relative values.

Authorised person to sign calibration reports is Mr. Marios Nicolaou.

General Remarks

The **Permanent Laboratory premises** are at the following address:
Democratias 5 Str, Ergates Industrial Estate, 2643 Nicosia, Cyprus.

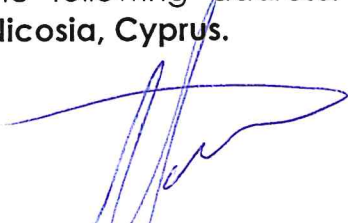

Antonis Ioannou
Director

Date: 20 October 2023